
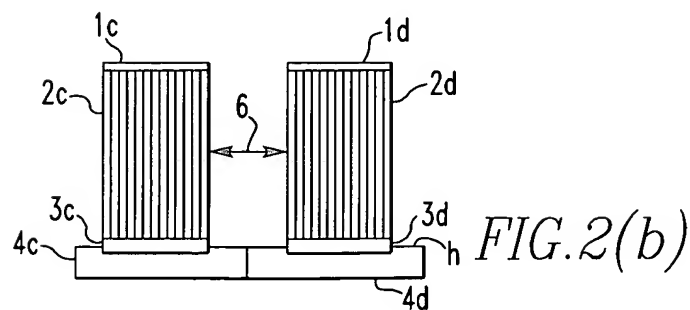
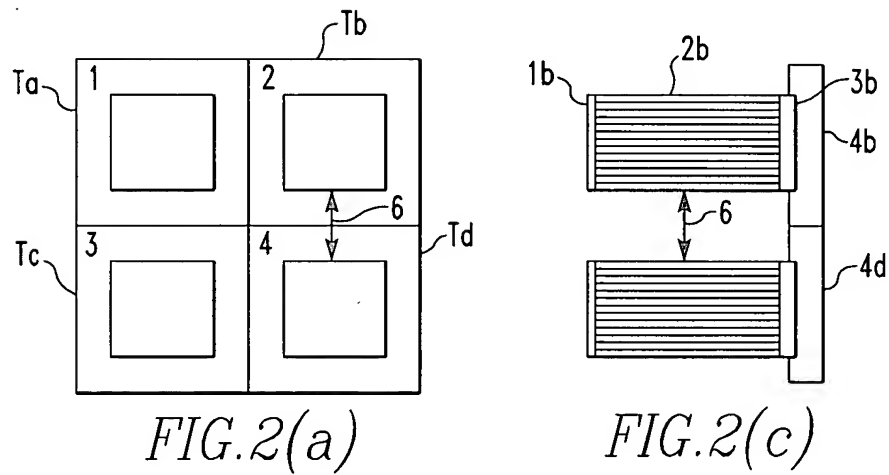


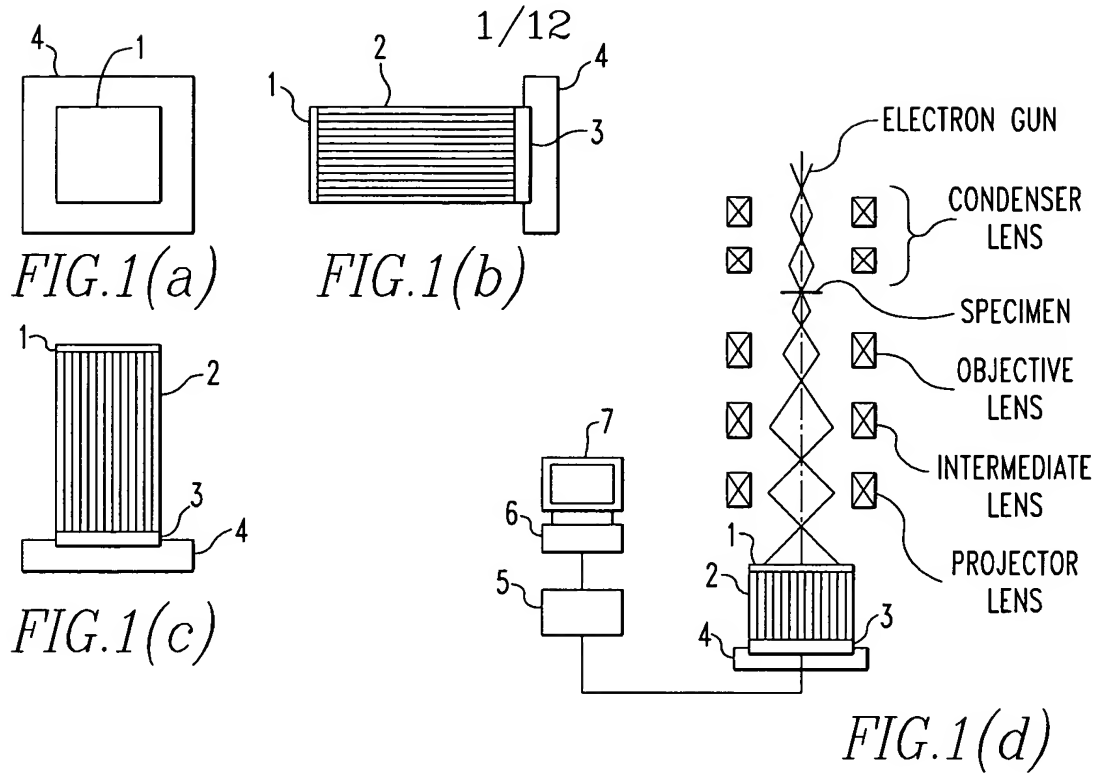


"Transmission Electron Microscope"

Application No. 10/678,956

Attorney Docket No. 116-031937



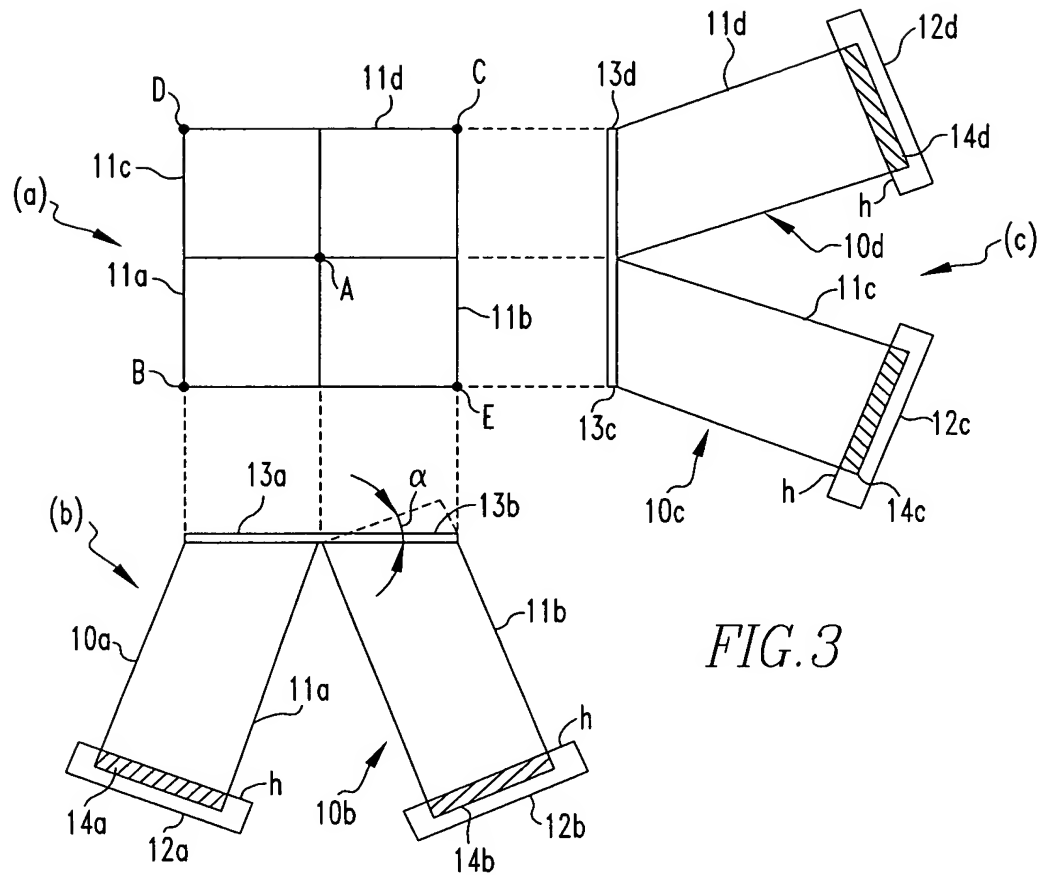

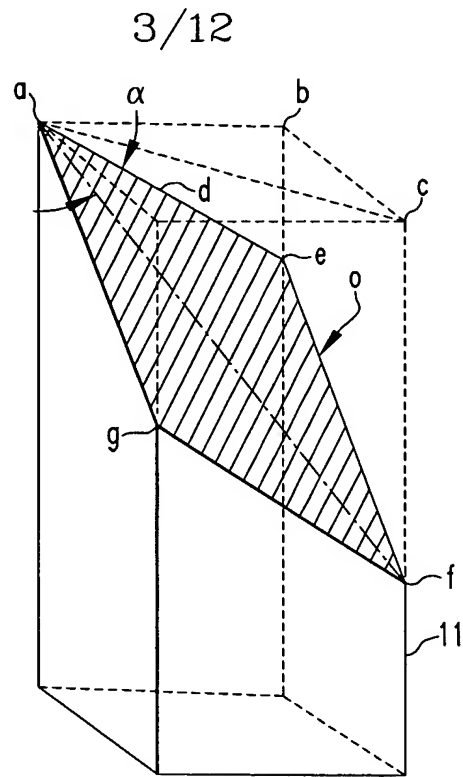


FIG. 4

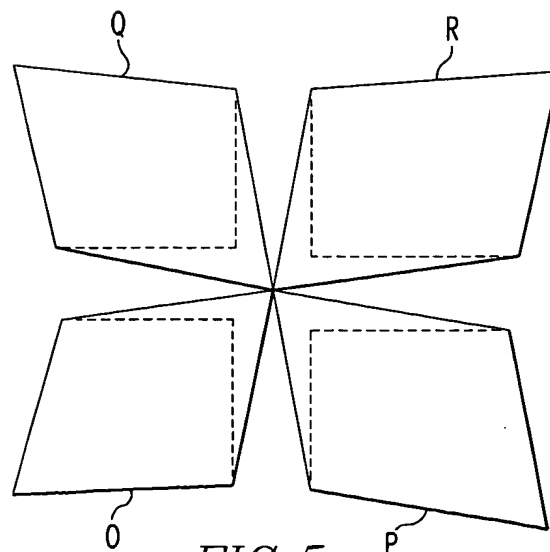


FIG. 5

4/12

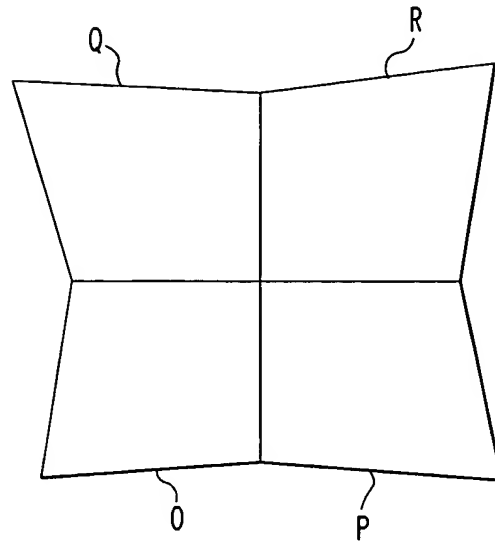


FIG. 6

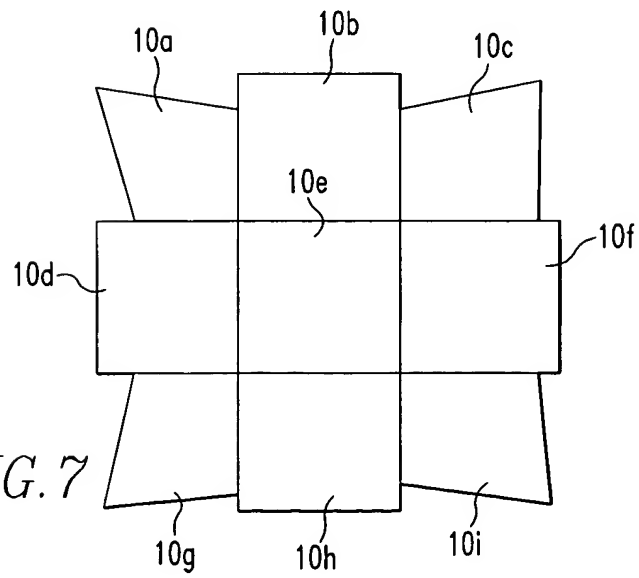


FIG. 7

5/12

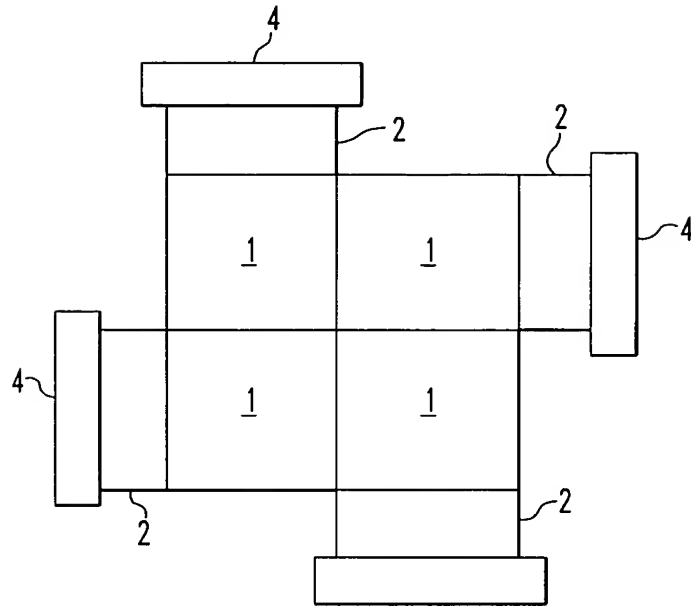


FIG. 8(a)

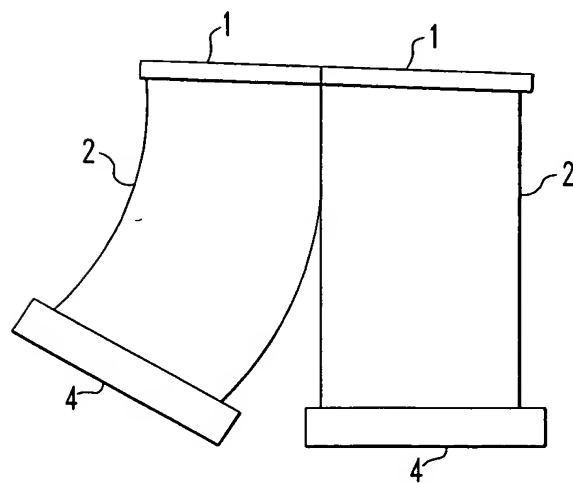


FIG. 8(b)

6/12

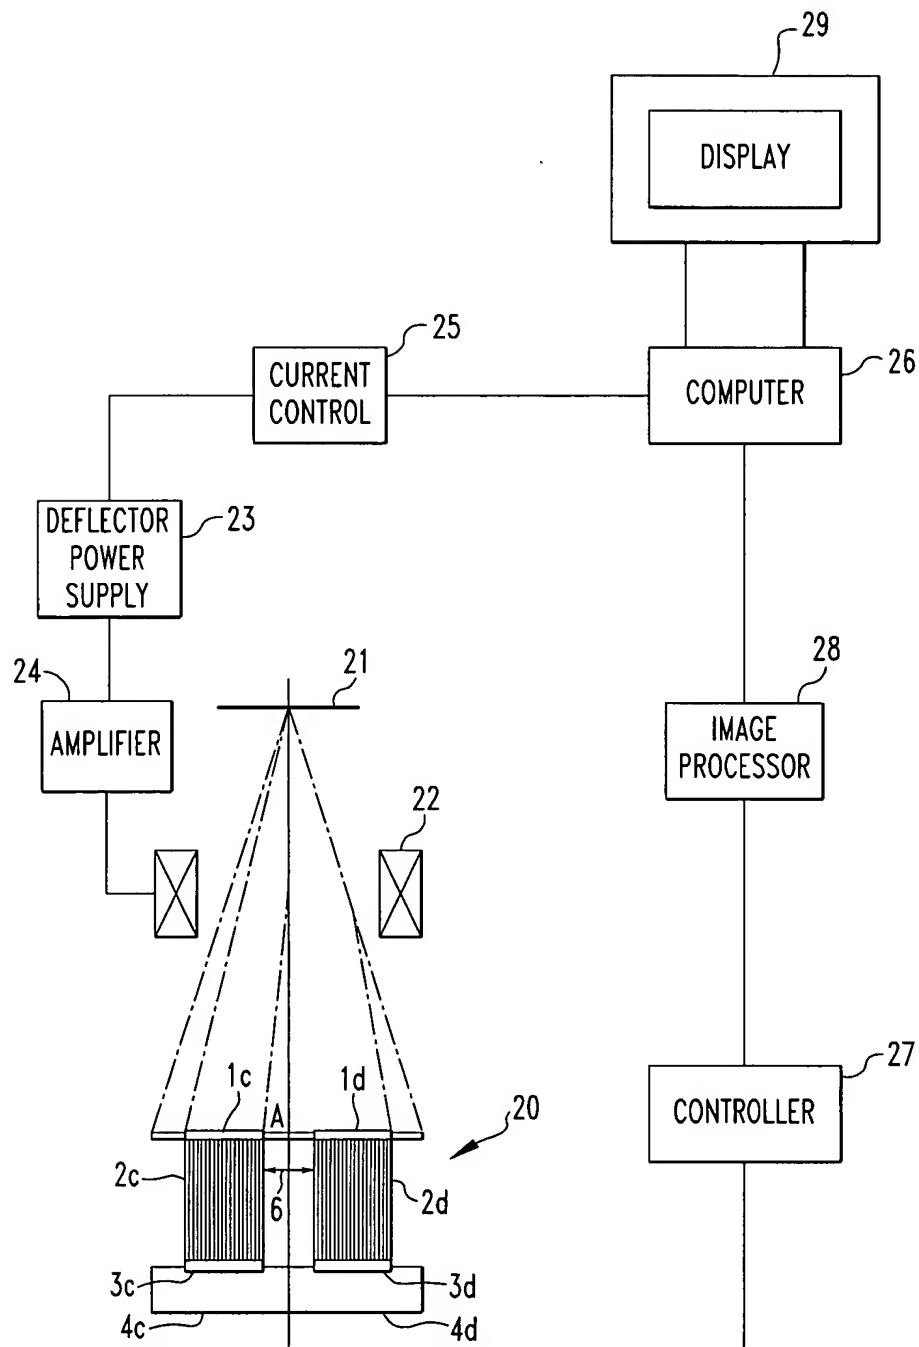


FIG. 9

7/12

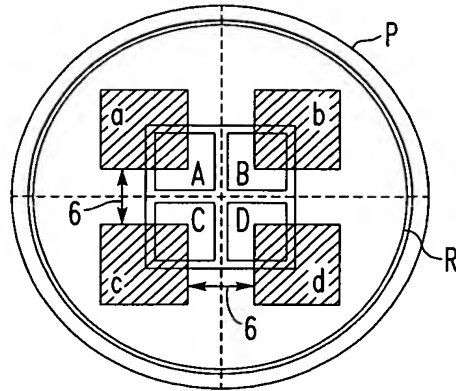


FIG. 10






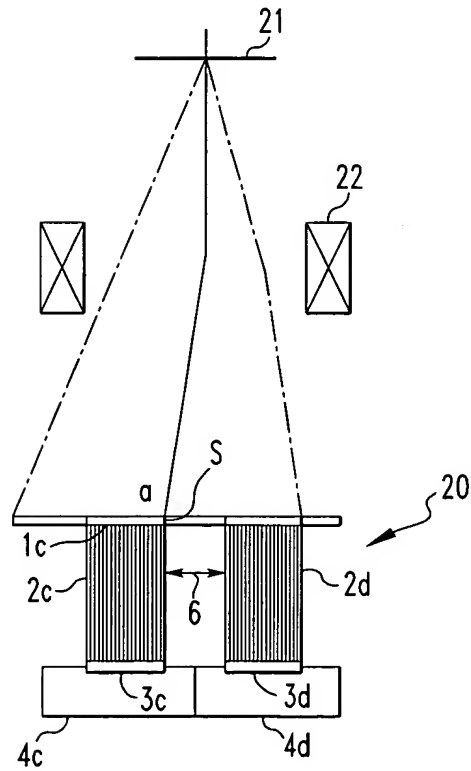


FIG. 12

8/12

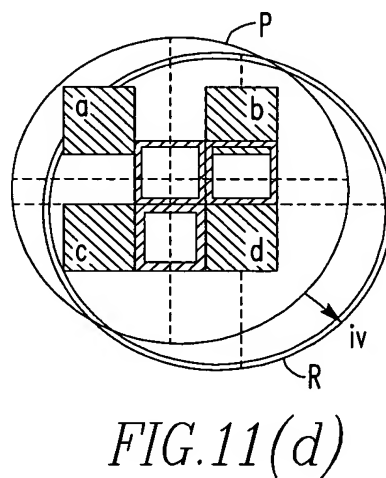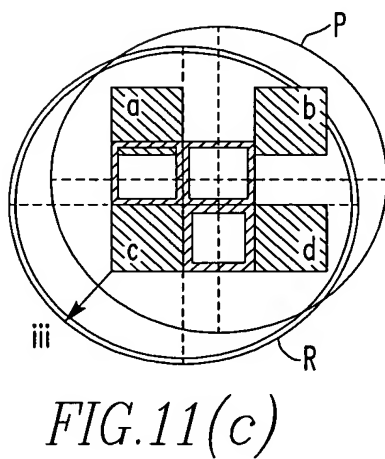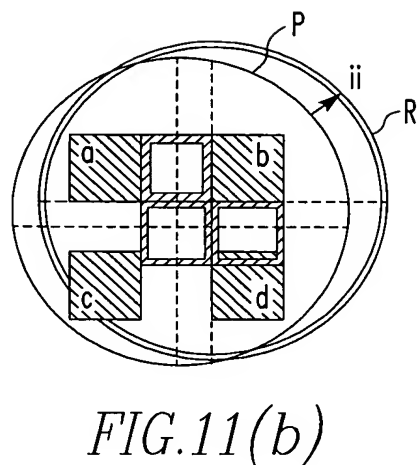

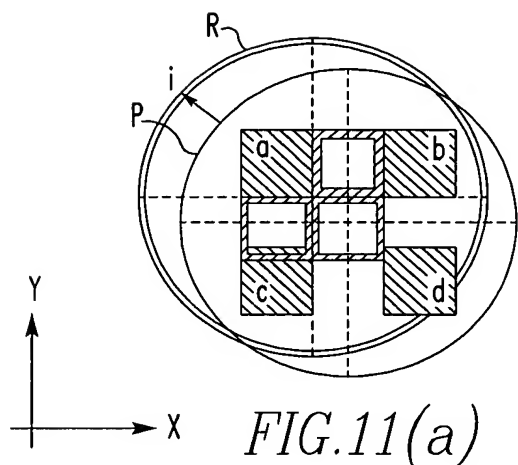

9/12

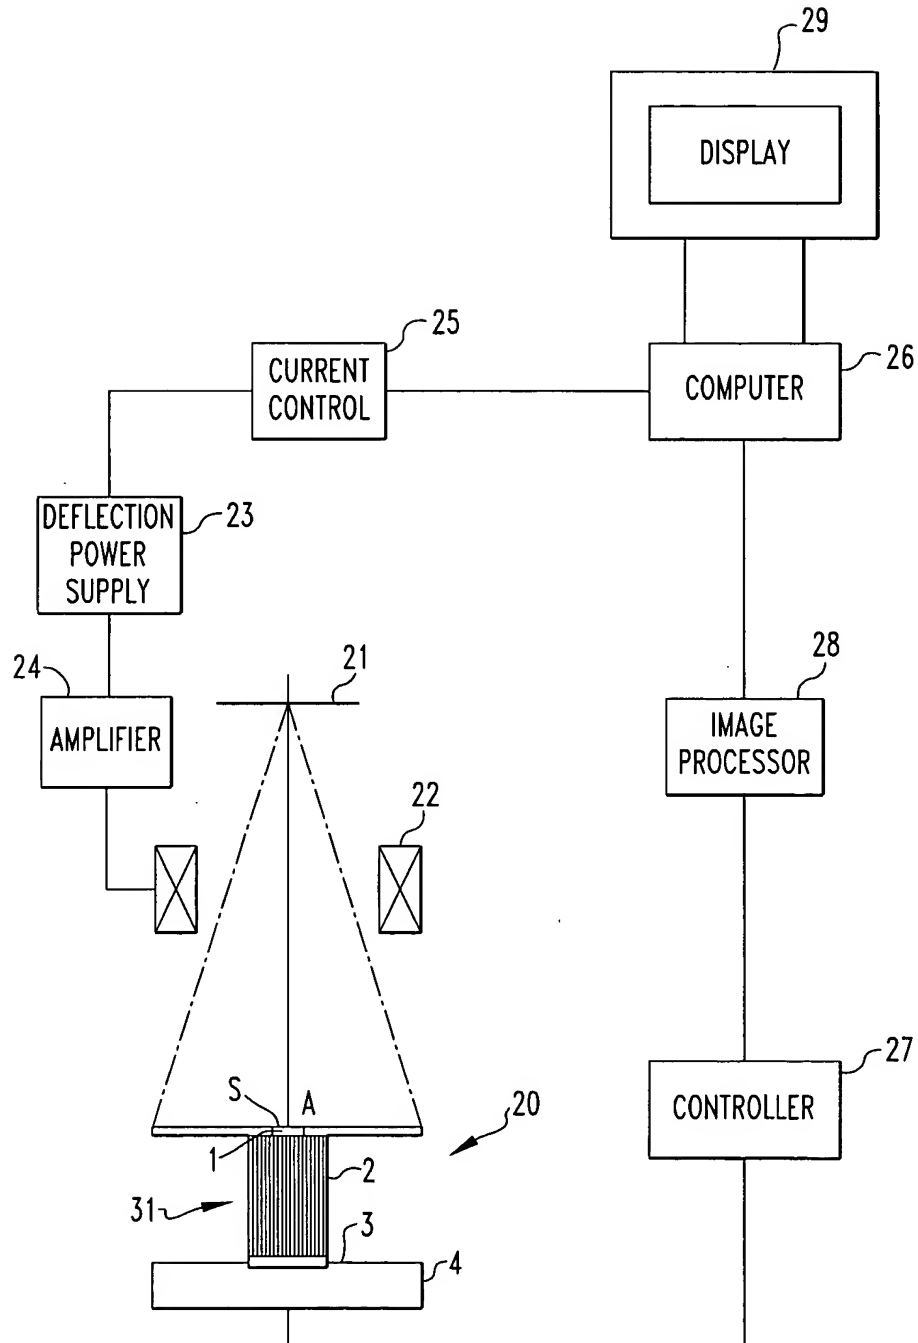
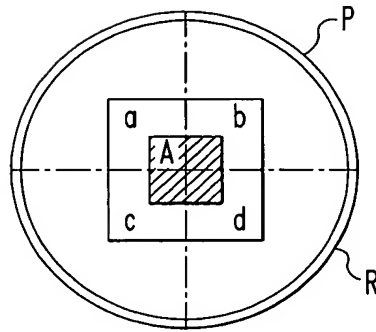


FIG.13

10/12



*FIG. 14*

11/12

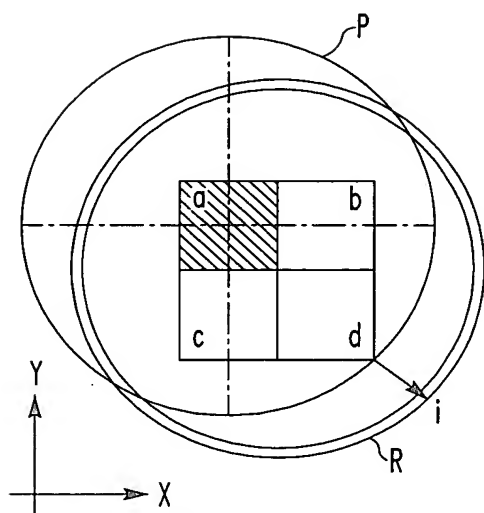


FIG. 15(a)

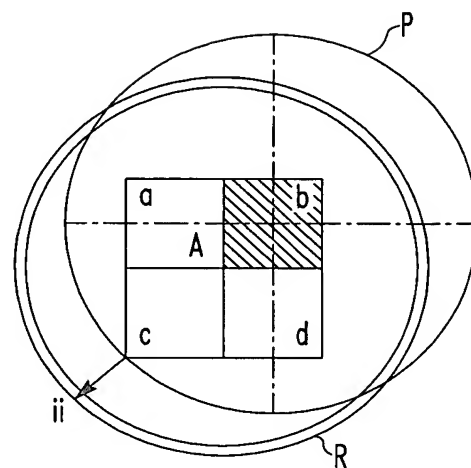


FIG. 15(b)

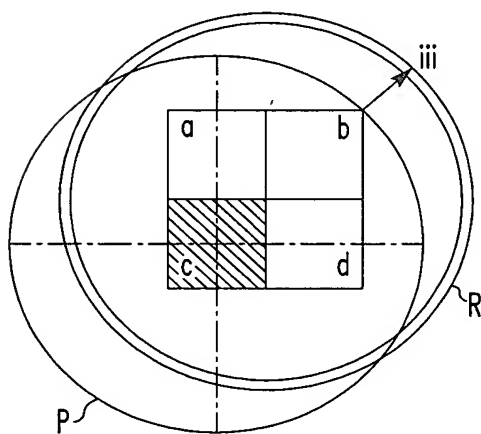


FIG. 15(c)

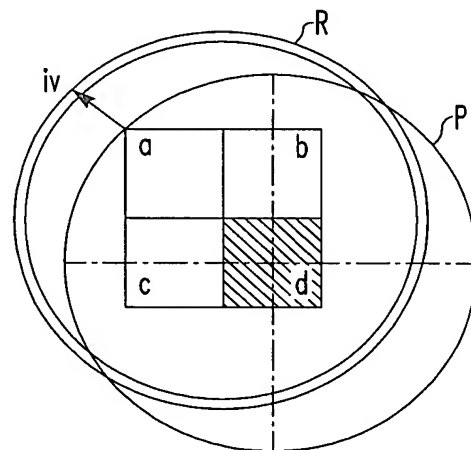


FIG. 15(d)




FIG. 15(e)

12/12

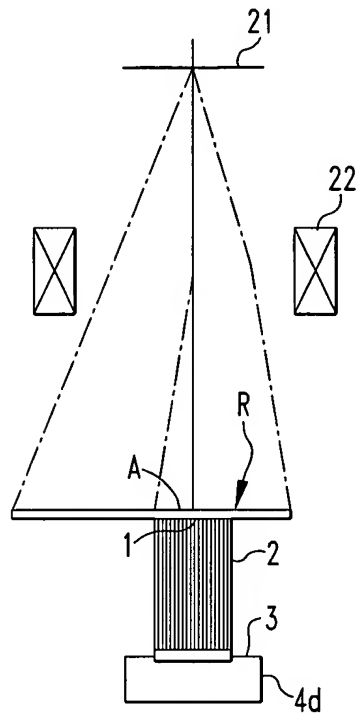


FIG.16